


500ml Basic Ozone Humidifier

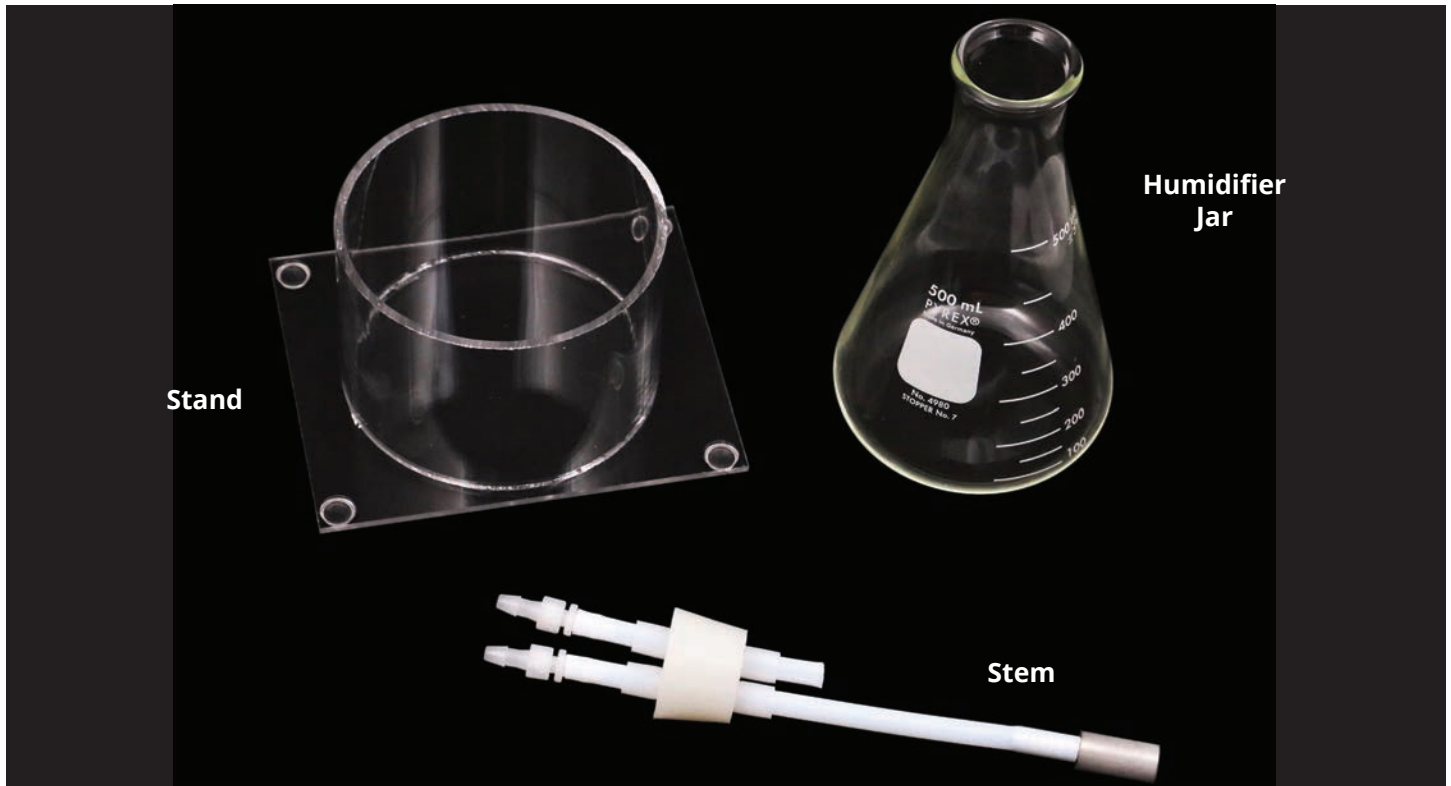

Fill the humidifier to at least the 200ml line on the jar (distilled water is best) and put the stem back in the jar. Place the humidifier into its stand.

Attach the end of a silicone tube coming from the Ozone Out on your ozone generator to the adapter provided on the left hand straw of your humidifier (the one that goes all the way into the humidifier).

Then attach the tubing coming from your earscope, catheter or other accessory to the right hand straw of the humidifier.

Allow the water to saturate for 2-5 minutes before using your earscope or catheter.